

REPORT OF EQUIPMENT CALIBRATION

INSTRUMENT DESCRIPTION

It is certified that the item under calibration has been calibrated by corresponding calibrated High Volume Sampler and the filter paper is weighted by HOKLAS laboratory.

Instrument: Handheld TSP meter

Brand Name: TSI
Model No.: AM520
Serial No.: 5201735004
Date of Calibration: 20 October, 2023
Date of Next Calibration: 20 October, 2024

ISSUING ORGANISATION

Address

Enovative Environmental Service Limited

Flat 23, 6/F, Block C, Goldfield Industrial Centre

1 Sui Wo Road Shatin, N.T. Hong Kong **Phone:** 852-2242 1020

Fax: 852-3691 9240 Email: info@eno.com.hk

and the sure of th




Brand Name: TSI
Model No.: AM520
Serial No.: 5201735004
HVS No.: A12-TSP-102
Date of Calibration: 20 October, 2023
Date of next Calibration: 20 October, 2024

Calibration Record

HVS - TSP (mg/m3)	0.0229	0.0330	0.0357	0.0349
TSI AM520 (mg/m3)	0.0238	0.0339	0.0369	0.0353

K Factor:	0.9961
Correlation Coefficient :	0.9969

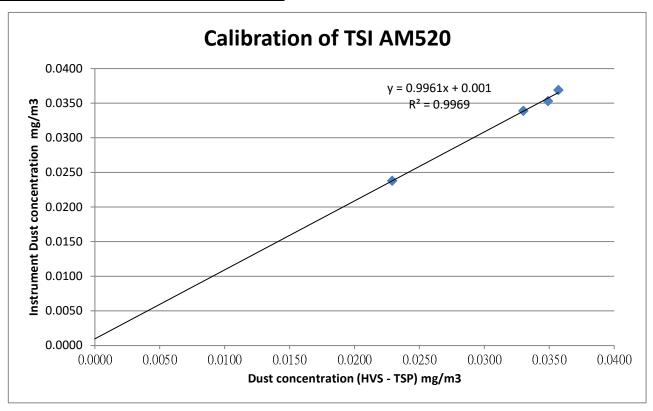

*** Filter paper being used in the calibration : 209591, 209592, 209593, 209594

Those filter papers are weighted by HOKLAS laboratory (ALS Technichem (HK) Pty Ltd.)

ENOVATIVE OF Thomas



REPORT OF EQUIPMENT CALIBRATION

INSTRUMENT DESCRIPTION

It is certified that the item under calibration has been calibrated by corresponding calibrated High Volume Sampler and the filter paper is weighted by HOKLAS laboratory.

Instrument: Handheld TSP meter

Brand Name: TSI
Model No.: AM520
Serial No.: 5201735006
Date of Calibration: 20 October, 2023
Date of Next Calibration: 20 October, 2024

ISSUING ORGANISATION

Address

Enovative Environmental Service Limited

Flat 23, 6/F, Block C, Goldfield Industrial Centre

1 Sui Wo Road Shatin, N.T. Hong Kong **Phone:** 852-2242 1020

Fax: 852-3691 9240 Email: info@eno.com.hk

andvarve of the small

Mr Wong Siu Ho, Thomas

Manager




Brand Name: TSI
Model No.: AM520
Serial No.: 5201735006
HVS No.: A12-TSP-102
Date of Calibration: 20 October, 2023
Date of next Calibration: 20 October, 2024

Calibration Record

HVS - TSP (mg/m3)	0.0229	0.0330	0.0357	0.0349
TSI AM520 (mg/m3)	0.0222	0.0339	0.0366	0.0346

K Factor:	1.0952
Correlation Coefficient :	0.9915

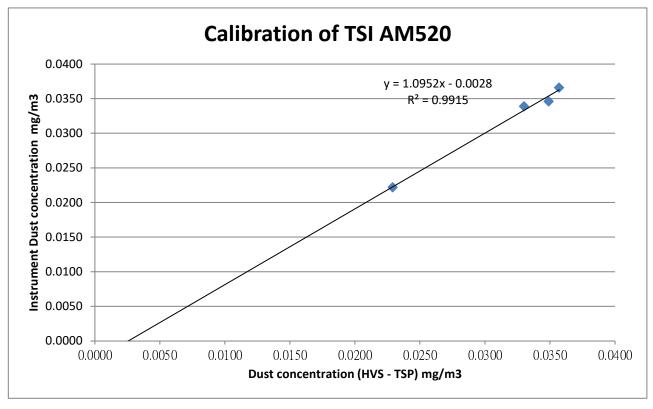

*** Filter paper being used in the calibration : 209591, 209592, 209593, 209594 Those filter papers are weighted by HOKLAS laboratory (ALS Technichem (HK) Pty Ltd.)

INDUSTRIES THOUSE OF THE STREET OF THE STREE



REPORT OF EQUIPMENT CALIBRATION

INSTRUMENT DESCRIPTION

It is certified that the item under calibration has been calibrated by corresponding calibrated High Volume Sampler and the filter paper is weighted by HOKLAS laboratory.

Handheld TSP meter Instrument:

Brand Name: AM520 Model No.: Serial No.: 5202345003 Date of Calibration: 21 January, 2024 Date of Next Calibration: 21 January, 2025

ISSUING ORGANISATION

Address

Enovative Environmental Service Limited

Flat 23, 6/F, Block C, Goldfield Industrial Centre

1 Sui Wo Road Shatin, N.T. Hong Kong

Phone: 852-2242 1020 Fax: 852-3691 9240

Email: info@eno.com.hk

homas

Mr Wong Siu Ho, Thomas

Manager




Brand Name: TSI
Model No.: AM520
Serial No.: 5202345003
HVS No.: A12-TSP-102
Date of Calibration: 21 January, 2024
Date of next Calibration: 21 January, 2025

Calibration Record

HVS - TSP (mg/m3)	0.0940	0.0451	0.0775	0.0307
TSI AM520 (mg/m3)	0.0988	0.0472	0.0745	0.0321

K Factor:	1.0123
Correlation Coefficient :	0.9882

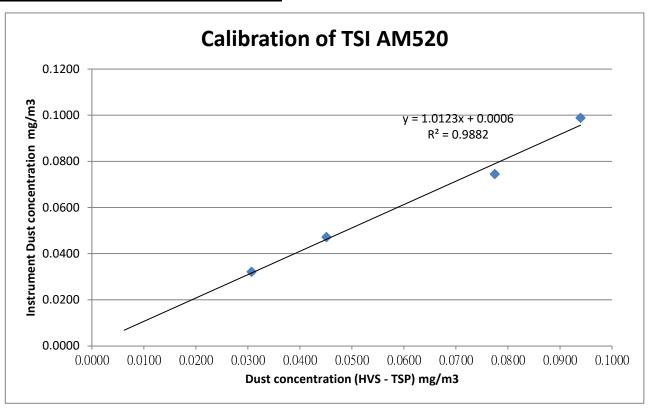

*** Filter paper being used in the calibration : 209603, 209604, 209605, 209606 Those filter papers are weighted by HOKLAS laboratory (ALS Technichem (HK) Pty Ltd.)

BNOVATIVE OF THE SURE STATE OF